

Certificate of Fitness

(Valid for 1 Year)

Construction Site ☐ Mining ☐ General ☒

Company : Ubhejane cranes

Name : S Dlamini

Date : 18/01/2018

Position : Technician

I.D.No: 6805056133081

Examination includes:

☒ Health Questionnaire and Physical examination

- Family Medical History
- Occupational History
- Abdomen
- Personal Medical History
- Physical Appearance
- Skin-Visual Acuity
- Tuberculosis
- Glandular/Endocrine
- Musculo-Skeletal
- Questionnaire
- Cardiovascular
- Medication

☒ Lung function test

☐ Baseline Audiogram

☒ Screening Audiogram

☐ Bronchodilator test

☒ TB Questionnaire

☒ X-Ray Chest

☐ Orthorator/Keystone

☒ L6/4 R6/5 Snellen Chart

☒ ECG

☒ Fields

☒ Colour Vision

☒ Depth perception

☐ Drug Testing

☒ Heat stress

☒ Work at Heights Evaluation

☐ K10 Stress Evaluation

Outcome of medical examination:

CERTIFICATION:	YES	NO	N/A	COMMENT/REASON:
Fit for work as per job description	x			
Fit to work at heights.	x			
Fit to drive Vehicle/Hyster			x	
Fit to work in hot conditions	x			
Fit for restricted work			x	
Temporarily unfit for work.			x	
Permanently unfit for work.			x	

Examiner/Physician Signature: 

Clinic Stamp: **Dr E M Liebenberg (MBBCh, DOH)**
WORKMED
PRACTICE NO.: 1440411
OIL & GAS UK: OGUK/2009/1349
SAMSA ACCREDITATION: MP0027/09
Southgate Business Park, Umbogintwini
P.O. Box 142, Umkomaas 4170
Tel: 031-914 4892 Fax: 031-914 4172

Print name: Dr E M Liebenberg (MBBCh, DOH) – Managing Director - WorkMed Group

Date of examination: 18/01/2018 Date of Expiry: 18/01/2019

Medical results Remarks:

PHYSICAL EXAMINATION


Employee Name : S Dlamini

ID Number : 6805056133081

NEUROLOGICAL ASSESSMENT

<u>Reflexes</u>	Present	Absent	Comments
A) Patella	x		
B) Ankle	x		
<u>Nystagmus</u>		x	
	Normal	Abnormal	
<u>Rombergs Test</u>	x		
<u>Appendicular coordination</u>			
A) Finger to nose	x		
B) Rapid Alternating hand movements	x		
<u>Gait</u>			
A) Normal	x		
B) Heel Toe	x		
<u>Visual Fields</u>	x		

Conclusions:

CERTIFICATION:	YES	NO	COMMENT/REASON:
Fit for work at heights as per job description	X		
Fit for restricted work			
Temporarily unfit for work.			
Permanently unfit for work.			
Physician's signature:  Double-Click to Sign	Official Company stamp: Dr EM Liebenberg (MBBCh, DOH) WORKMED PRACTICE NO.: 1440411 OIL & GAS UK: OGLUK/2009/1349 SAMSA ACCREDITATION: MP0027/09 Southgate Business Park, Umbogintwini P.O. Box 142, Umkomas 4170 Tel: 031-914 4892 Fax: 031-914 4172		
Physician's name and qualifications:	Dr EM Liebenberg (MBBCh, DOH)		

Date of examination: 18/01/2018	Date Of Expiry: 18/01/2019
---------------------------------	----------------------------

Step Test – Physical Work Capacity (Heat Stress Evaluation)

Employee name: Sipho Dlamini Initials S.E. Sex: ☒ M / ☐ F
ID No: 6805056133081 D.O.B: 05/05/68 Age: 49
Occupation/Job title: Crane Technician Work Load Heavy
Company: Ubhejane Cranes Tel No: _____
Address: _____ Date: 18/1/18

History

Previous test: ☒ Y / ☐ N History of chest pain on exertion: ☒ Y / ☐ N Previous coronary episode: ☒ Y / ☐ N

If **YES** then date of episode: _____

Dyspnoea: ☒ Y / ☐ N History of Cardiac disease: ☒ Y / ☐ N

Current medication: NIL

Recent illness or hospitalisation: NIL

History of heat disorder: ☒ Y / ☐ N Date: _____

Respiratory problems including asthma: NIL

Remarks: _____

Employee Signature: _____

Examination

Height: 181.5 Weight: 103.7 Urine test: NAD

Blood sugar if indicated: N/A Body/Mass Index: _____

Initial BP Seated: 140/85 Pulse Rate: 74 Regular: yes

Oedema: ☒ Y / ☐ N Cyanosis: ☒ Y / ☐ N Skeletal abnormality: NAD

Pulse rate after 10 mins of exertion: 150/90 B.P: 86

Work Capacity: ☒ Heavy / ☐ Medium / ☐ Light Date of Test: 18/1/18

Fit to work in hot conditions: ☒ X / ☐ N Remarks _____

Expiry Date: 18/1/19

Examiners' signature: _____

Print name: E.M. Liebenberg

Designation: O.M.P.

Company Stamp
WORKMED
PRACTICE NO: 1440411
OIL & GAS UK: CGUK/2009/1349
SANSI ACCREDITATION: MP0027/09
Southgate Business Park, Umbogintwini
P.O. Box 142, Umkomas 4170
Tel: 031-914 4662 Fax: 031-914 4172

Employee Details

Employee 680505 MR EMMANNEUL SIPHO DLAMINI Mal
Birth date 1968-05-05 (49) Employed on - -
Department Company MORRIS MAT HANDLING
Biological M Occupation TECHNICIAN
Next Test 2020-01-17 Aux/ID. 680505 6805056133081

Brief Audiogram History DLAMINI ES 680505

Date	TYP	.5K	1K	2K	3K	4K	6K	8K	.5K	1K	2K	3K	4K	6K	8K	Cat	PLH	PLH-Sh	PBI	
2010-06-01	1415	SC	05	10	15	25	10	15	20	05	10	15	20	20	10	AA	1	1.6	?	0.0
2016-01-06	0843	SC	15	15	20	25	15	20	00	10	20	20	25	25	15	10	1	2.6	?	0.0
2017-01-23	0923	SC	10	10	20	25	25	15	10	05	15	15	25	25	15	05	1	2.2	?	0.0

BL-Baseline SC-Screening MO-Monitoring DI-Diagnostic
CO-Compensation BC-Baseline Comparison EX-Exit


Deterioration from Baseline DLAMINI ES 680505

Date	TYP	.5K	1K	2K	3K	4K	6K	8K	.5K	1K	2K	3K	4K	6K	8K	PLH	DETER	
Baseline or Compensation audiograms not found.																		
2018-01-18	1544	SC	10	15	20	25	25	15	05	05	20	20	25	30	15	10	3.0	?

BL-Baseline SC-Screening MO-Monitoring DI-Diagnostic
CO-Compensation BC-Baseline Comparison EX-Exit

Screening Audiogram DLAMINI ES 680505 2018-01-18 154

PLH: 3.0% PLH Shift from Baseline: ?% Deterioration: ?dBHL Ear: Freq:
CAT:2 PBI: 0.0% RTS:10 Ear:Lt Freq:4K ABHL:17.50

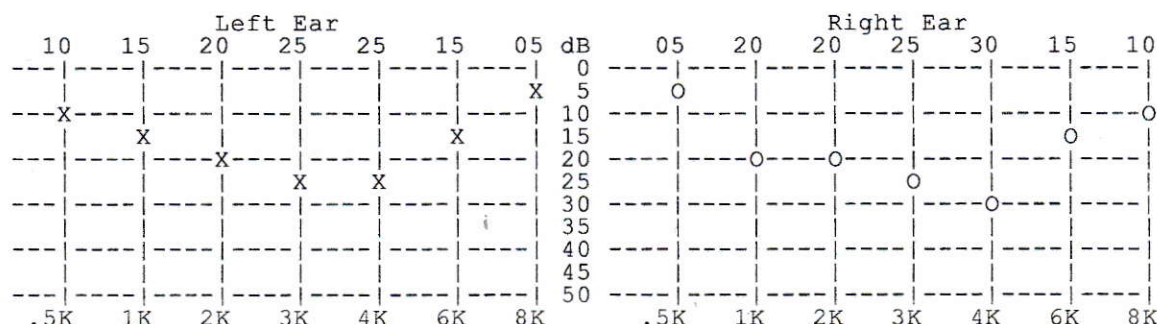

Company :MORRIS MAT HANDLING
Biological:

Department:
Occupation:TECHNICIAN

Tested by Supervisor: *Q. Robins*
Tremetrics RA300 Audiometer #2220

Employee's acceptance
Calibration Date: 1701

Employee Notes

-- End of document --

Dr EM Liebenberg (MBBCh, DOH)
WORKMED
PRACTICE NO.: 1440411
OIL & GAS UK: OGUK/2009/1349
SAMSA ACCREDITATION: MP0027/09
Southgate Business Park, Umbogintwini
P.O. Box 142, Umkomas 4170
Tel: 031-914 4892 Fax: 031-914 4172



Lung Function Test Details WORKMED - UMBOGINTWINI

2018-01-18 15:54

IJEBW115: cli

Patient Number:	680505	Gender & Ethnic:	Male / African	Company:	MORRIS MAT HANDLING
Patient Name:	DLAMINI, EMMANNEUL SIPH	Height & Weight:	1.81 m / 103 kg (31.44)	Department:	
Identity No:	6805056133081	Smoker:	No	Position:	TECHNICIAN
Date of Birth:	1968-05-05	Asthma:	No	Service:	
Test Date:	2018-01-18	Test Time:	15:53:53	Operator:	clinic
Predicted Ref:	ERS/ECCS * 0.9	Session Quality:	=?	Acceptable:	2/3
Reproducible:	Yes	Variability:	FEV1 0.08L 2.20%, FVC 0.06L 1.23%		
Interpretation:					
Calibration:	Easy on-PC	Calibration Time:	2018-01-18 08:14:44	Room Temperature:	25.30 deg C
Spirometer S/N:	222233	Operator:	clinic	Barometric Pressure:	1,010.00 mm Hg
Syringe Serial No:	2007SY485	Syringe Volume:	3.00 L	Relative Humidity:	51.00 %

Parameter	Pred	Trial 2	Trial 1	Trial 3	Pred %
Acceptable	-	Yes	Yes	No	-
FVC (L)	4.33	4.70	4.38	4.64	108.54
FEV1 (L)	3.48	3.73	3.46	3.64	106.91
FEV1/FVC (%)	78.30	79.26	78.98	78.49	98.50
PEF (L/s)	9.16	10.44	9.19	10.08	114.07
FEF 25-75 (L/s)	4.10	3.34	3.12	3.21	81.41
FEF 75 (L/s)	2.11	1.35	1.17	1.18	63.97
FEF 50 (L/s)	4.99	4.19	3.79	3.98	84.00
FEF 25 (L/s)	7.99	7.30	7.41	8.24	91.39
FET	-	6.04	5.64	5.95	-

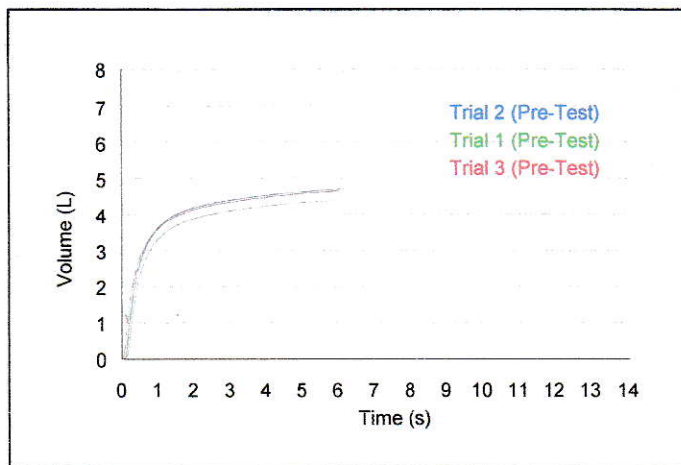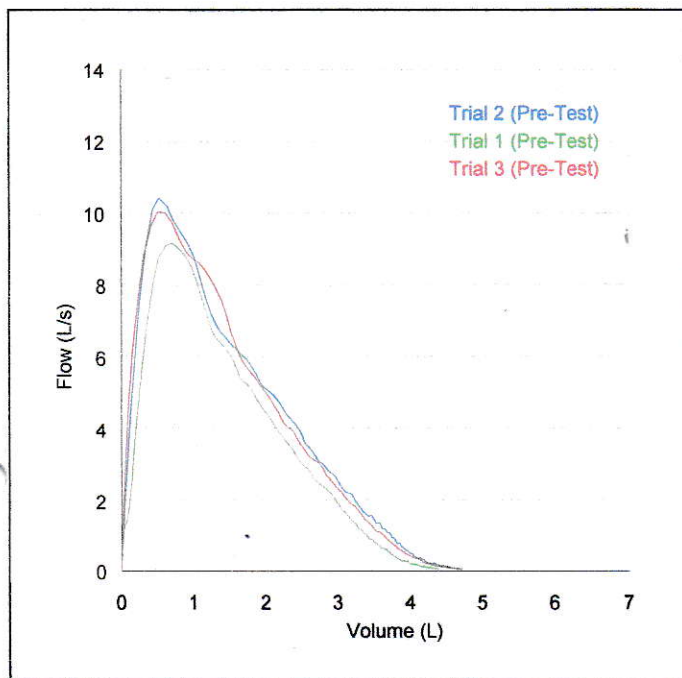

Notes

Acknowledgement >>

Operator:

[Signature]

Date:

18/1/18

Patient:

[Signature]

Date:

18/1/18

Dr EM Liebenberg (MBBCh, DOH)
WORKMED
PRACTICE NO.: 1440411
OIL & GAS UK: OGUH/2005/1349
SAMSA ACCREDITATION: MP0027/09
Southgate Business Park, Umbogintwini
P.O. Box 142, Umkomas 4170
Tel: 031-914 4392 Fax: 031-914 4172



Dr. Zemfundo Portia Malevu Inc.

MbChB (Natal) FcRad (Diag) SA

T/A Kwadukuza Radiology Services

SPECIALIST RADIOLOGISTS

PR. No: 0594997

Patient : MR SIPHO DLAMINI
Date of Birth : 05/05/1968
Examination Date : 18/01/2018
Referring Doctor : DR LEIBENBERG
Reference Number: INV11-2272
Centre : MZANSI XRAY

CHEST X RAY

1. The lung fields are clear with no confluent areas of air-space opacification or evidence of infiltrative disease.
2. The hilar regions are normal in appearance, location and density.
3. The cardiac silhouette is within the normal limits.
4. The diaphragmatic outlines are crisp and smooth.
5. There is no obliteration of the costo-phrenic angles.
6. There are no obvious soft tissue and bone abnormalities.

Comment:

THERE IS NO EVIDENCE OF PULMONARY TUBERCULOSIS.

Reported by: DR ZP MALEVU

Dr EM Liebenberg (MBCh, DOH)
WORKMED
PRACTICE NO.: 1440411
OIL & GAS UK: OGUK/2009/1349
SAMSA ACCREDITATION: MP0027/09
Southgate Business Park, Umbogintwin
P.O. Box 142, Umkomaas 4170
Tel: 031-914 4092 Fax: 031-914 4172

Contrast 226 167 02

CE 0459

LOT D 976

MAC 500

U2.23

GEMS-IT

18. Jan. 18 15:56

GEMS-IT

18. Jan. 18 15:56

Serial Number: 510003712

Last Name

Diamini

First Name

SE

Date of Birth



6805056133081

Sex


M

Measurement Results:

QRS : 84 ms
QT/QTc : 364 / 401 ms
PR : 168 ms
P : 132 ms
RR/PP : 818 / 820 ms
P/QRS/T : 40/ 50/ -6 Degrees



Auto 25mm/s 10mm/mV ADS

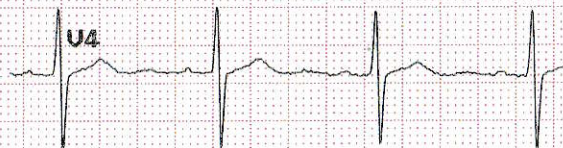

50Hz 0,08-35Hz 72BPM

MAC 500

U2.23

12SL U 13